

HPLC Analysis for RG7388




=====
Acq. Operator : SYSTEM
Acq. Instrument : 12601c

Seq. Line : 8
Location : Vial 93

Inj Volume : 2.000 µl

Additional Info : Peak(s) manually integrated

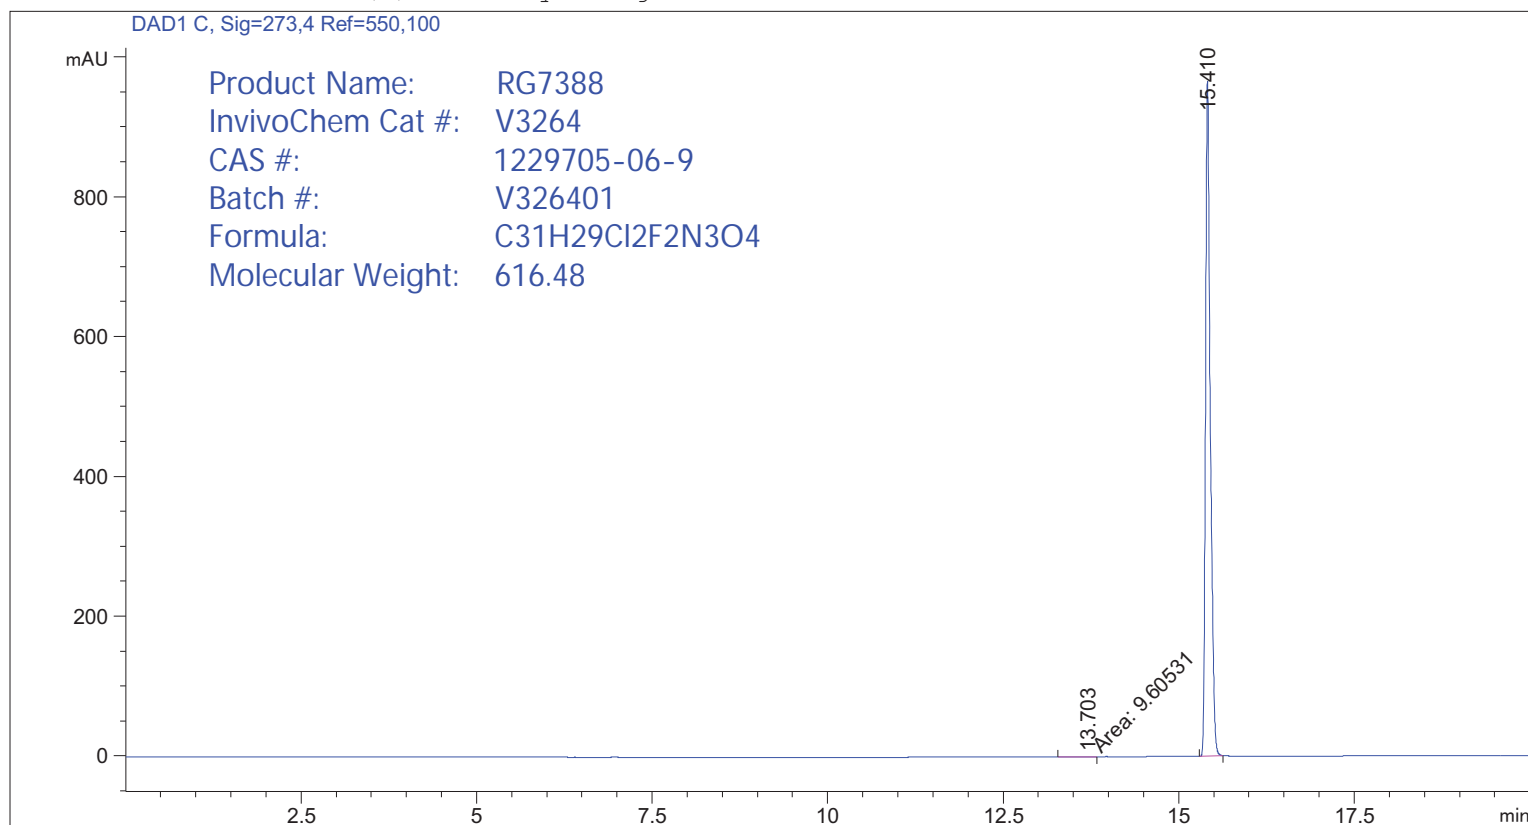

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 C, Sig=273,4 Ref=550,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	13.703	MM	0.3613	9.60531	4.43099e-1	0.2099
2	15.410	BB	0.0692	4566.96875	965.39618	99.7901

Totals : 4576.57406 965.83928

=====
*** End of Report ***