HPLC Analysis for BLU9931

```
-----------------------------------------------------------------------
Acq. Operator   : SYSTEM                          Seq. Line :   3
Acq. Instrument : LC1260                           Location :   P1-F2
Injection Date  : 6/29/2016 9:17:10 AM                  Inj :   1
                                                 Inj Volume : 5.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 3.000 µl
Acq. Method     : D:\Chem32\1\Data\2016\201606\Analysis 2016-06-29 08-42-25\10-80_CD.254.M
Last changed    : 6/29/2016 8:42:26 AM by SYSTEM
Analysis Method : C:\Chem32\1\Methods\wash.M
Last changed    : 6/30/2016 4:14:52 PM by SYSTEM
```

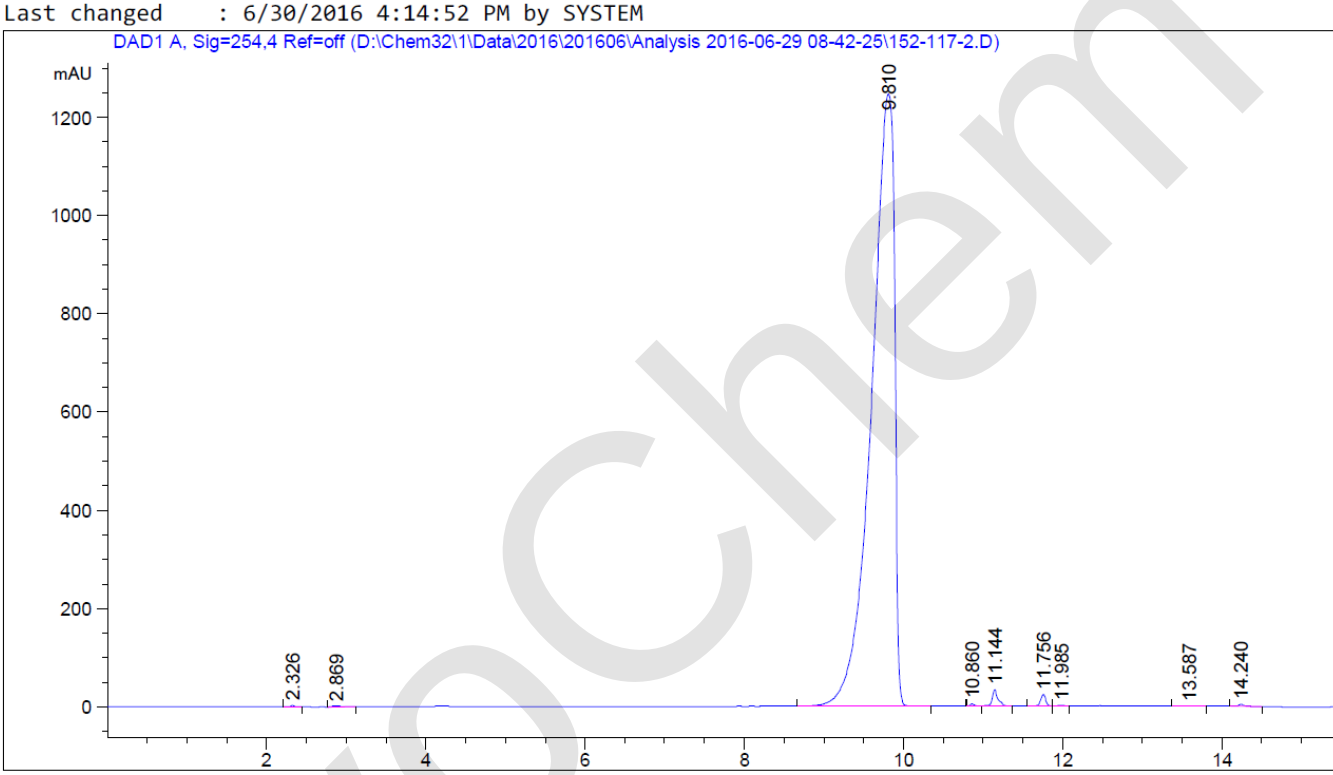


```
=======================================================================
                        Area Percent Report
=======================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=254,4 Ref=off
```

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	2.326	BV	0.0500	7.48138	2.29937	0.0297
2	2.869	BB	0.1047	14.17893	2.10325	0.0563
3	9.810	BB	0.3025	2.48516e4	1247.21545	98.6126
4	10.860	BV E	0.0587	16.75978	4.57657	0.0665
5	11.144	VB R	0.0730	170.68590	33.77263	0.6773
6	11.756	BV	0.0701	104.34372	23.34927	0.4140
7	11.985	VB	0.0891	8.22423	1.47456	0.0326
8	13.587	BB	0.1003	7.14818	1.09314	0.0284

InvivoChem

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
9	14.240	BB	0.0631	20.81663	4.75726	0.0826

Totals : 2.52012e4 1320.64150

==========

*** End of Report ***

InvivoChem