
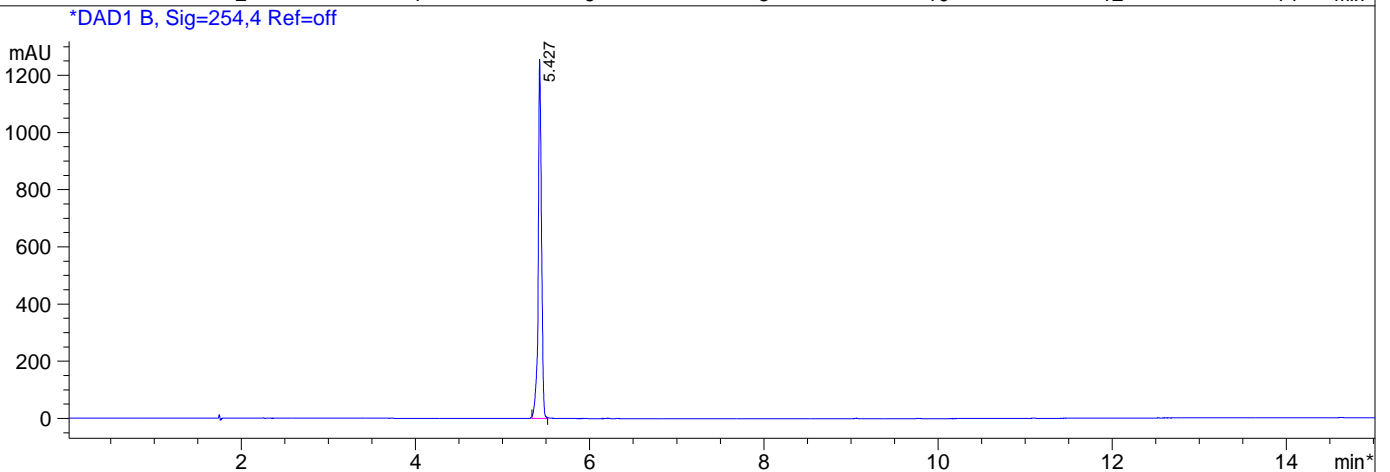


File D:\DATA\
 Injection Date : 01-Jun-16, 18:19:09 Tgt Mass(EZX) :
 Sample Name : Location :
 Acq. Operator : Inj : 0
 Spec. Reported : MS Integration Inj Volume : 2 ul
 Acq. Method : D:\METHODS\2-HPLC.M
 Analysis Method : D:\METHODS\2-HPLC.M
 Sample Info : Easy-Access Method: '2-HPLC.M'
 Method Info : Column:Xbridge C18 (4.6x150 mm, 3.5um)
 Mobile phase: H2O(10 mmol NH4HCO3) (A) / ACN(B)
 Elution program: Gradient from 5 to 95% of B in9min at 1ml/min
 Temperature:50°C
 Detection: UV (214 , 4 nm) and MS (ESI, Neg mode ,70 to 900 amu)

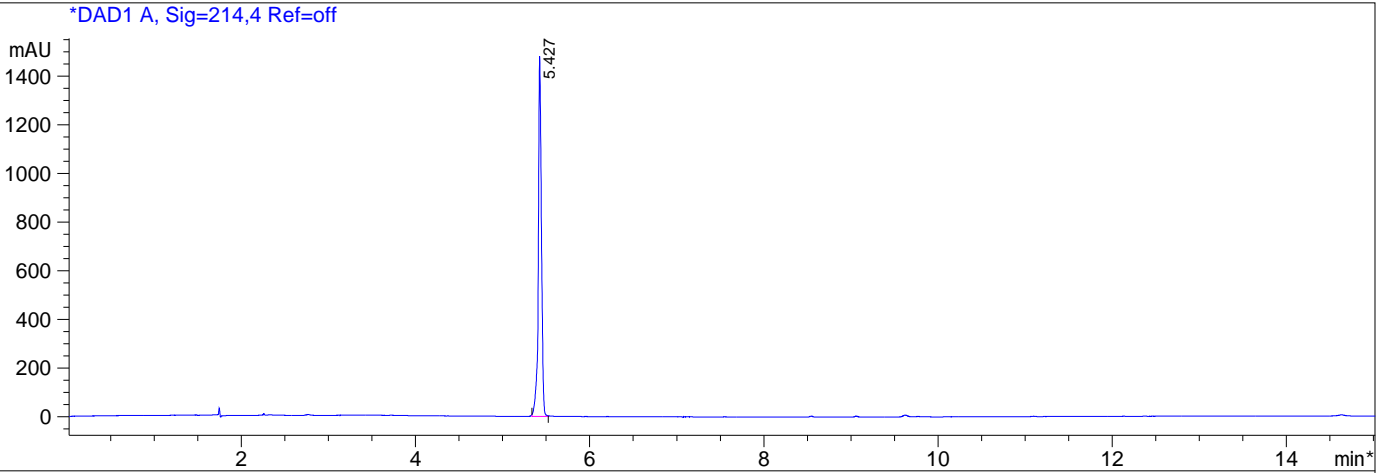

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
5.43	0.04	3689.76	1436.09	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
5.43	0.04	3276.96	1221.29	100.00