
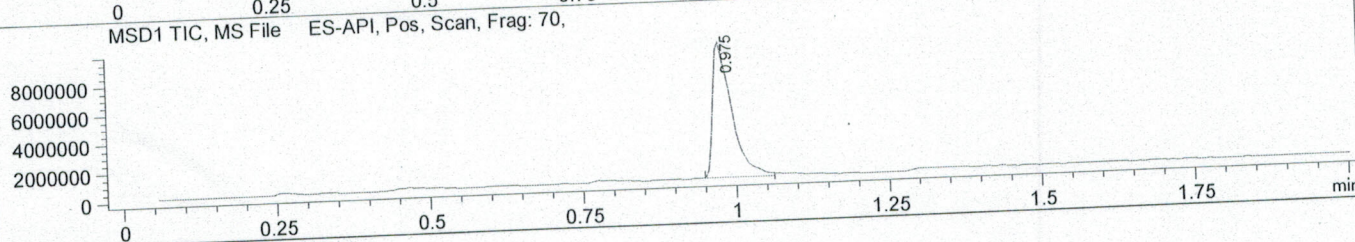
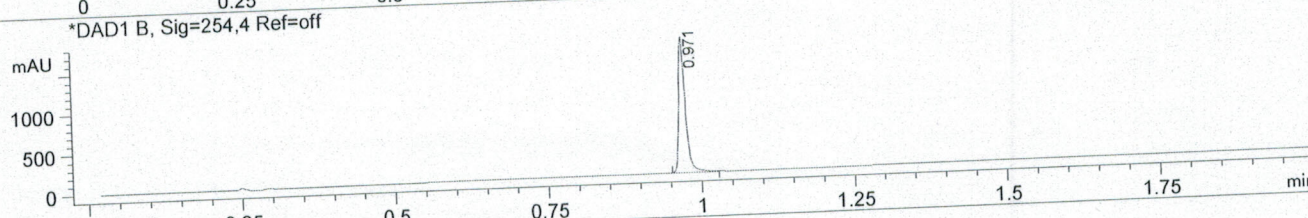
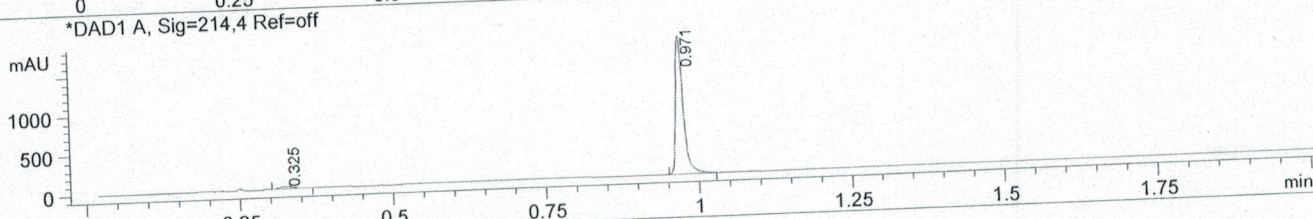


File D:\DATA
 Injection Date : 7 Nov 14 3:45
 Sample Name : 161814-49-9
 Acq. Method : C:\Chem32\1\METHODS\1-POS-2MIN.M
 Analysis Method : C:\Chem32\1\METHODS\1-POS-2MIN.M
 Sample Info : Easy-Access Method: '1-POS-2MIN'
 Method Info : Mobile Phase: A: Water(0.01%TFA) B: ACN(0.01%TFA)
 Gradient: 5%B increase to 100%B within 0.8min,100%B for 1.1min.
 Flow Rate:1.5mL/min
 Column: Chromolith Fast Gradien RP-18e,50-3mm.
 Column Temperature: 40C
 Mass Range:103-1100

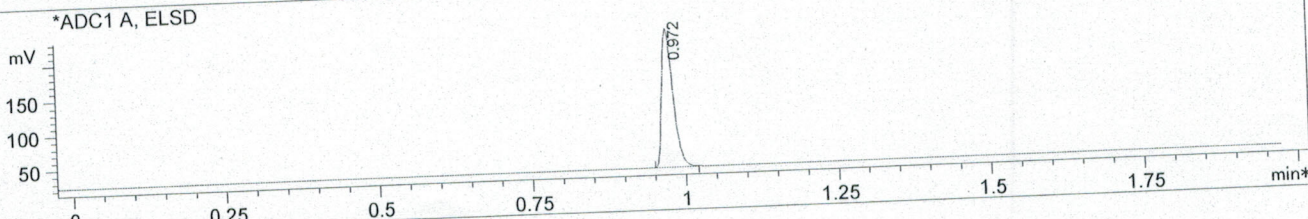

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
0.97	0.02	258.39	200.60	100.00

Integration Results for DAD1 A, Sig=214.4 Ref=off

RetTim	Width	Area	Height	Area%
0.32	0.02	43.49	29.64	2.79
0.97	0.01	1517.11	1767.49	97.21

Integration Results for DAD1 B, Sig=254.4 Ref=off

RetTim	Width	Area	Height	Area%
0.97	0.01	1294.12	1703.76	100.00

Ret. Time: 0.97

<<<< POSITIVE SPECTRA >>>>

