

HPLC Analysis for Protein degrader 1 HCl

Data File: c:\gilson\unipoint\pro2019.025\pro2019.gdt

Date acquired: Mon Jul 1 2019 11:24:36

Control Method: C:\GILSON\UNIPOINT\SYSTEM.GCT

Analysis Method: C:\GILSON\UNIPOINT\SYSTEM.GAN

Sample name: ULM-1

Sample site: Sample:4

Injection Number: 8 *Unknown*

Channel Scales

<Auto range Analysis Channel>

214 0.00 to 10.00 mVolt (0 %offset), Data rate: 20.00 (points/second)

<Auto zero> <Analysis Channel>

254 0.00 to 10.00 mVolt (5 %offset), Data rate: 20.00 (points/second)

<Auto zero>

Peak Table

<None>

Peak Detection Parameters

Relative Error: 5 (%) Absolute Error: 0.1 (min)

Product Name: Protein degrader 1 HCl


InvivoChem Cat #: V4063

CAS #: 1448189-80-7

Batch #: V406301

Formula: $C_{22}H_{31}ClN_4O_3S$

Molecular Weight: 467.02

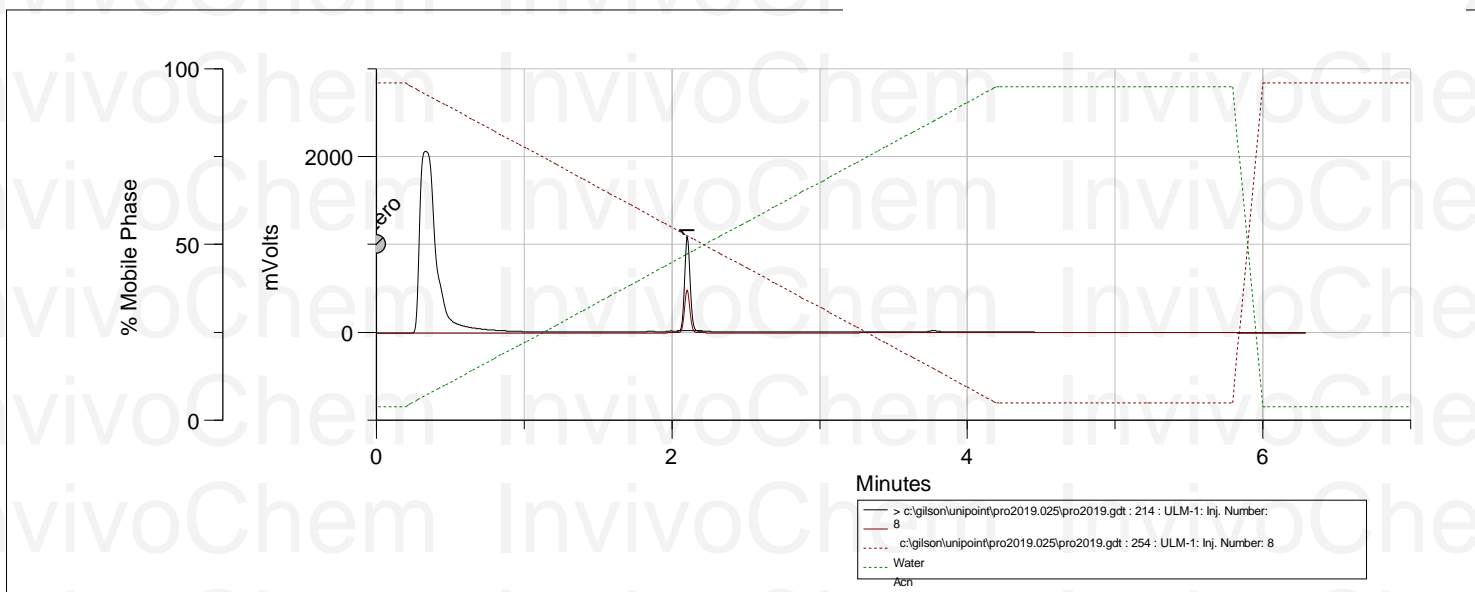

	Inj. Number	Peak Name	Sample Descrip.	R. Time	Sample Location	Height	Area	Area %		
1	8.00	1		2.10	Sample:4	1067.50	4567978.50	100.00		