^{1}MS Analysis for Vasotide

MS Spectrum

Positive

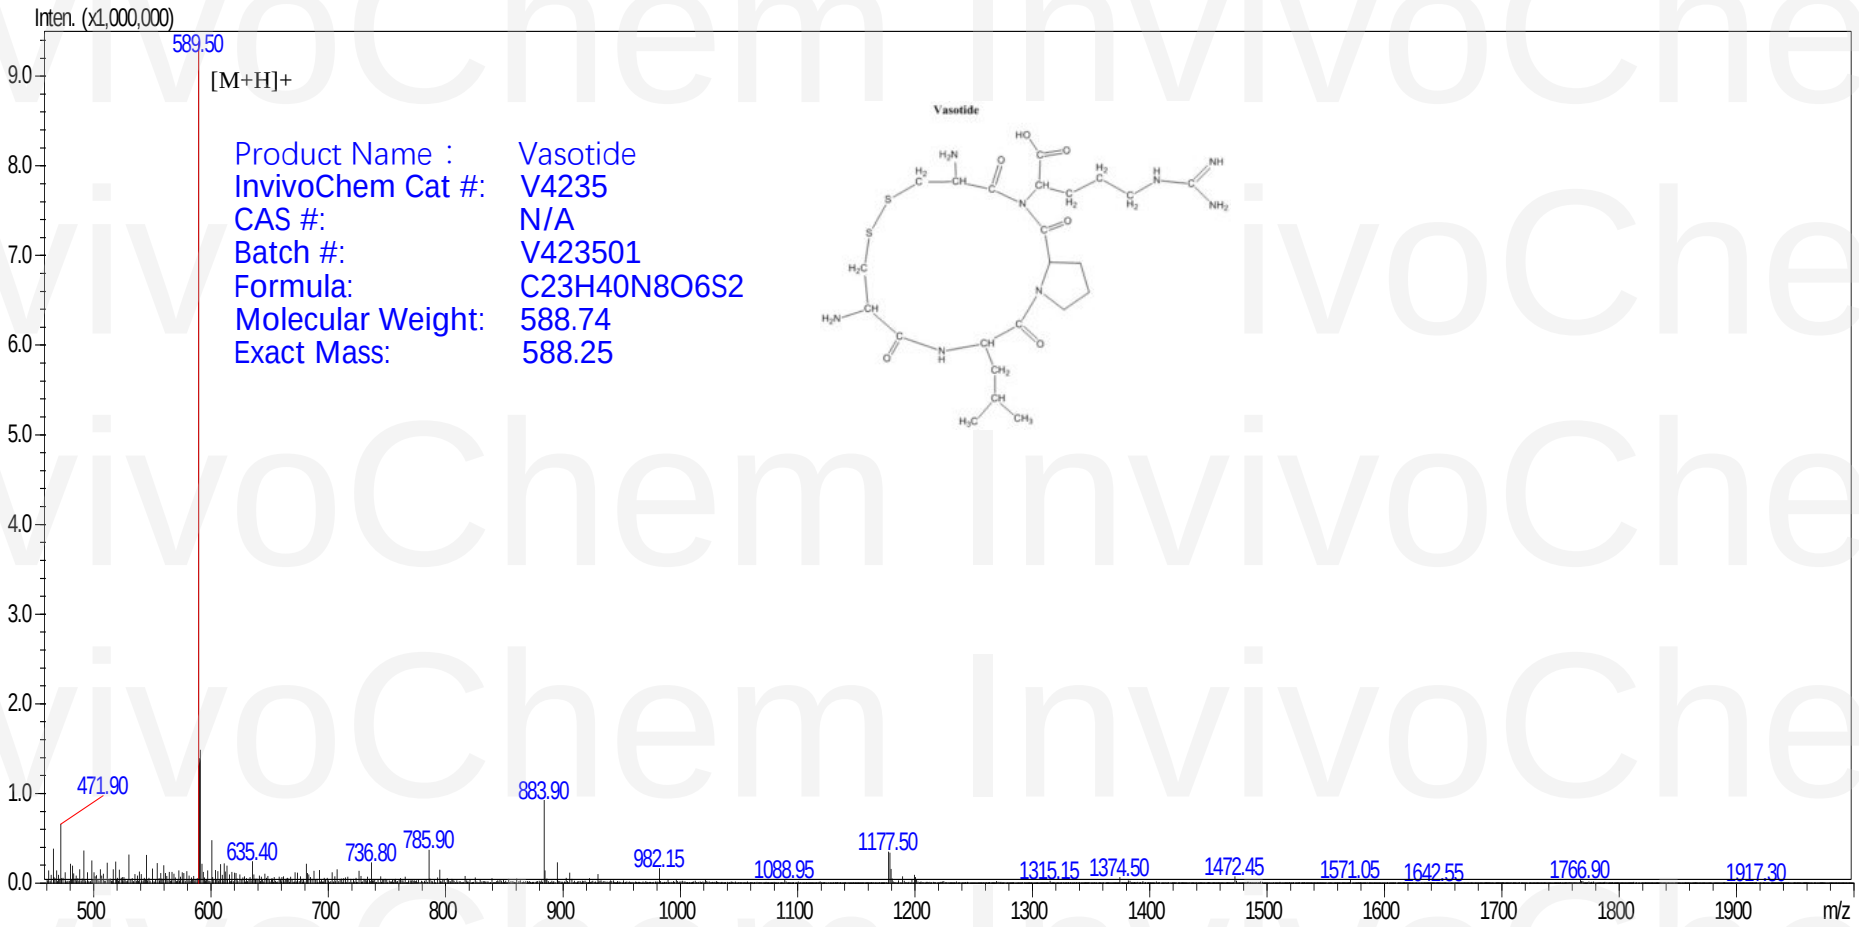

Acquired by :Shen
Data Acquired : 2019/6/3
Injection Volume : 1
Sample Name : Vasotide CC-5
Mw : 588.74
Lot No. : P190513-CQ726104

Probe	:ESI	Probe bias	:+4.5kv
Nebulizer Gas Floe	:1.5L/min	Detector	:1.2kv
CDL	:-20.0v	T.Flow	:0.2ml/min
CDL Temp	:250℃	B.conc	:50%H2O/50%ACN
Block Temp	:400℃		