

HPLC Report

Sample name: xljt

Sequence:

Mobile phase: A: 0.1% TFA in H2O


B: 0.1% TFA in ACN

Gradient: 24-44%B in 20min Flow rate: 1.0ml/min

Column: Welch, C18, 4.6*150mm, 5um

Inject Date: 02/06/2018

Inj.Vol: 10uL

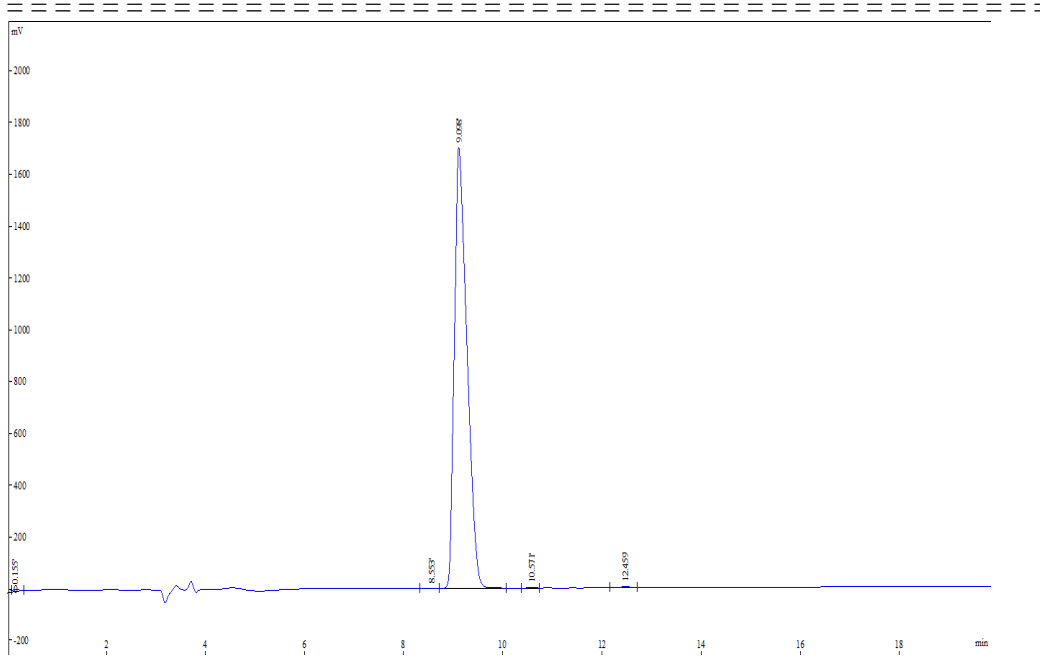

Area Percent Report

VWD: 220nm

Results

Pk#	Retention Time	Area Percent(%)	Area
1	0.007	0.2371	71086
2	0.155	0.2807	84131
3	8.553	0.03032	9089
4	9.098	99.22	29742093
5	10.571	0.03004	9005
6	12.459	0.2037	61062
Total		100	29976466