


## 1. Analysis Information

Product Name:	BLZ945
Operator:	David
Injection Date:	11/16/2017 7:52:46 PM
Batch No.:	4

## 2. HPLC Condition

Column:	Athena C18, 3 $\mu$ m, 2.1mm $\times$ 100 mm																
Solvent A:	0.1% H3PO4 in 100% Acetonitrile																
Solvent B:	0.1% H3PO4 in 100% Water																
Gradient:	<table border="1"> <thead> <tr> <th>Time</th> <th>A</th> <th>B</th> </tr> </thead> <tbody> <tr> <td>0.0min</td> <td>5%</td> <td>95%</td> </tr> <tr> <td>9.0min</td> <td>95%</td> <td>5%</td> </tr> <tr> <td>15.0min</td> <td>95%</td> <td>5%</td> </tr> <tr> <td>15.0min</td> <td>Stop</td> <td>Stop</td> </tr> </tbody> </table>		Time	A	B	0.0min	5%	95%	9.0min	95%	5%	15.0min	95%	5%	15.0min	Stop	Stop
Time	A	B															
0.0min	5%	95%															
9.0min	95%	5%															
15.0min	95%	5%															
15.0min	Stop	Stop															
Flow rate:	0.4ml/min																
Wavelength:	210nm																
Volume:	10 $\mu$ l																

## 3. Result

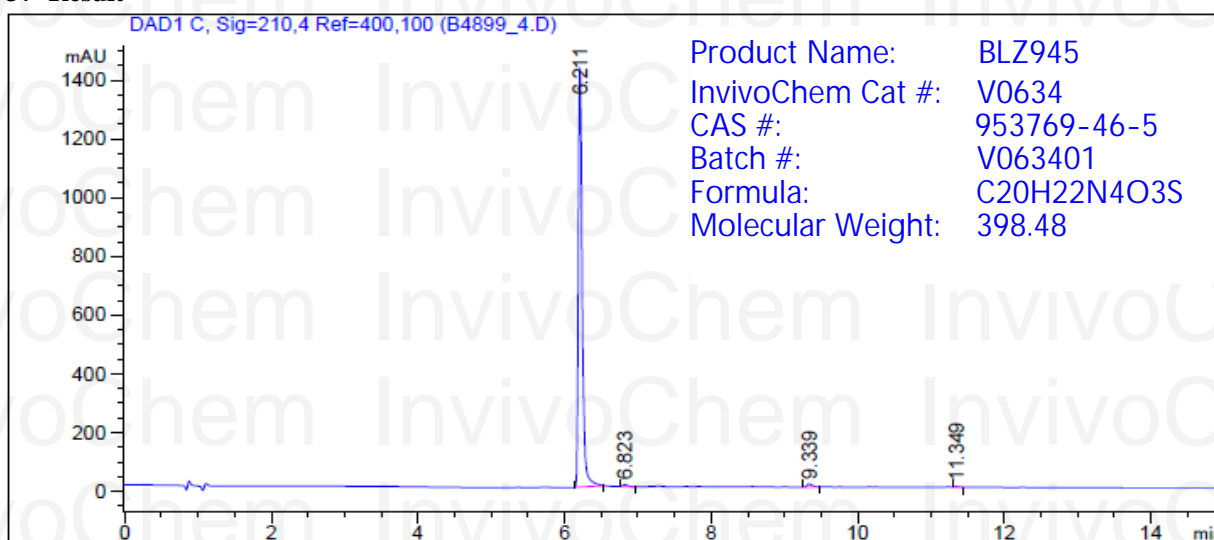

Rank	RetTime(min)	Area(mAU*s)	Area %
1	6.211	5281.19385	98.3018
2	6.823	32.86157	0.6117
3	9.339	50.85856	0.9467
4	11.349	7.51248	0.1398