


# V060901 Entrectinib HPLC

=====  
Acq. Operator : SYSTEM  
Acq. Instrument : 12601c

Seq. Line : 1  
Location : Vial 81

Inj Volume : 2.000 µl  
Different Inj Volume from Sample Entry! Actual Inj Volume : 2.500 µl

Additional Info : Peak(s) manually integrated

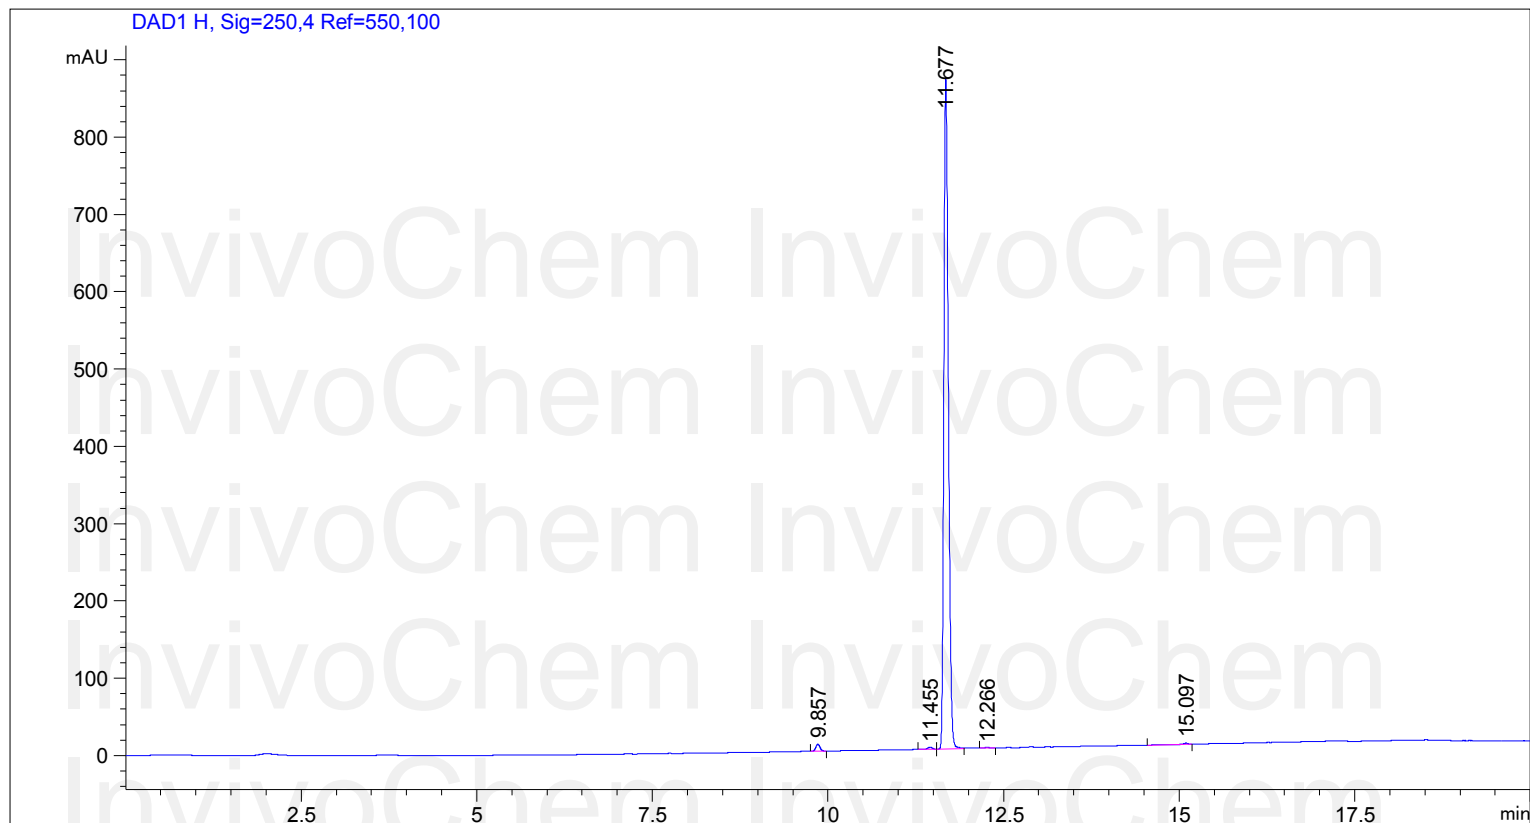

=====  
Area Percent Report  
=====

Sorted By : Signal  
Multiplier : 1.0000  
Dilution : 1.0000  
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 H, Sig=250,4 Ref=550,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	9.857	BB	0.0644	17.60175	4.05675	0.4582
2	11.455	BB	0.0754	4.74541	1.06606	0.1248
3	11.677	BV	0.0689	3858.79419	866.58936	99.0299
4	12.266	BB	0.0710	5.17935	1.09856	0.1320
5	15.097	BB	0.0814	7.01237	1.16029	0.1551

Totals : 3924.33307 881.07102