


V320001 NCB-0846 HPLC

=====
Acq. Operator : SYSTEM
Acq. Instrument : 12601c

Seq. Line : 1
Location : Vial 40

Inj Volume : 2.000 µl

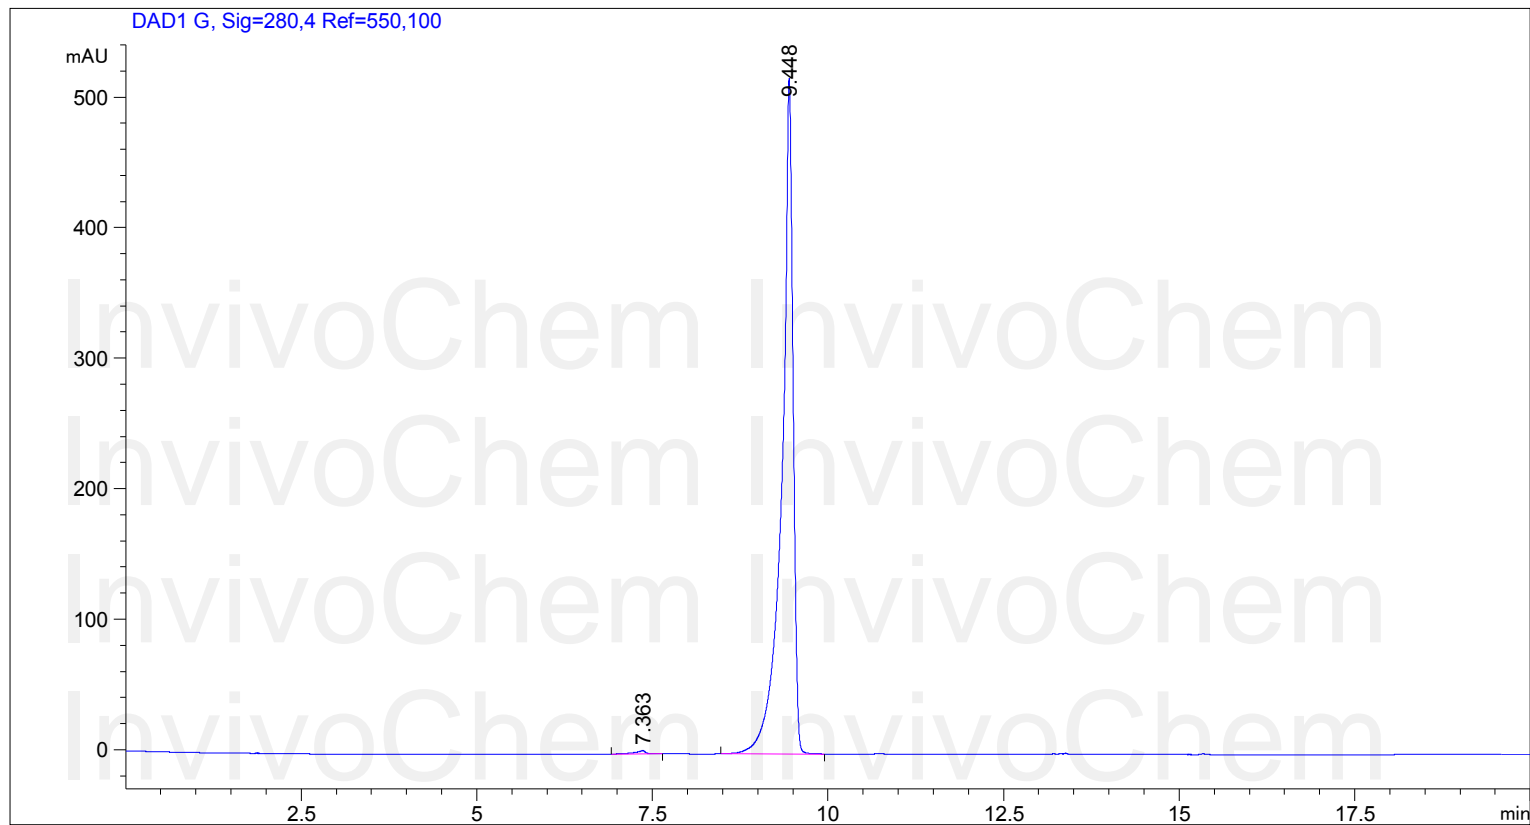

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 G, Sig=280,4 Ref=550,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	7.363	BB	0.1445	27.41709	2.53892	0.4752
2	9.448	BB	0.1509	5741.76367	517.68024	99.5248

Totals : 5769.18077 520.21916

=====
*** End of Report ***