
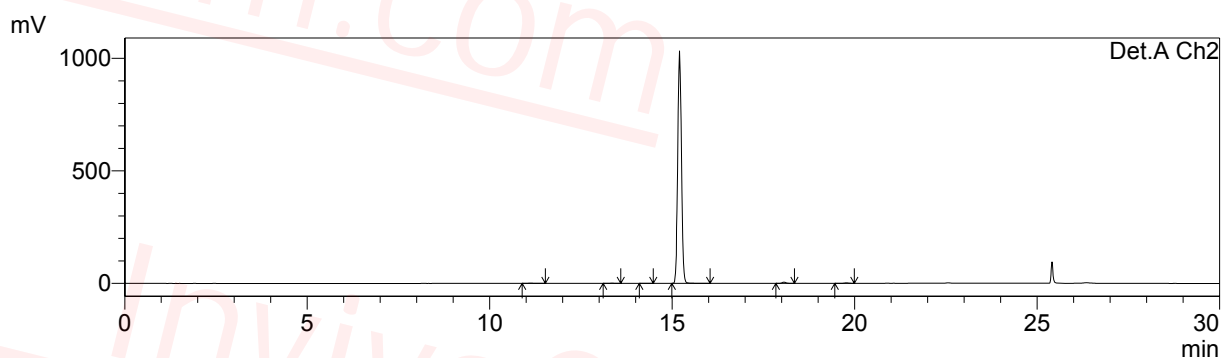


HPLC Report

Column : Diamonsil C18(2), 5um 4.6*250mm
Mobile phase : Solvent A: H2O(0.05%H3PO4) Solvent B:ACN(0.05%H3PO4)
Temperature : 35 °C
Flow rate : 0.8mL/min
Run time : 6min gradient(5%B), 9min gradient (5%-95%B), 5min gradient (95%B),then 5min @(5%B)
Detector : UV
Wavelength : 220/280 nm
User name : 116793
Sample name : 116793

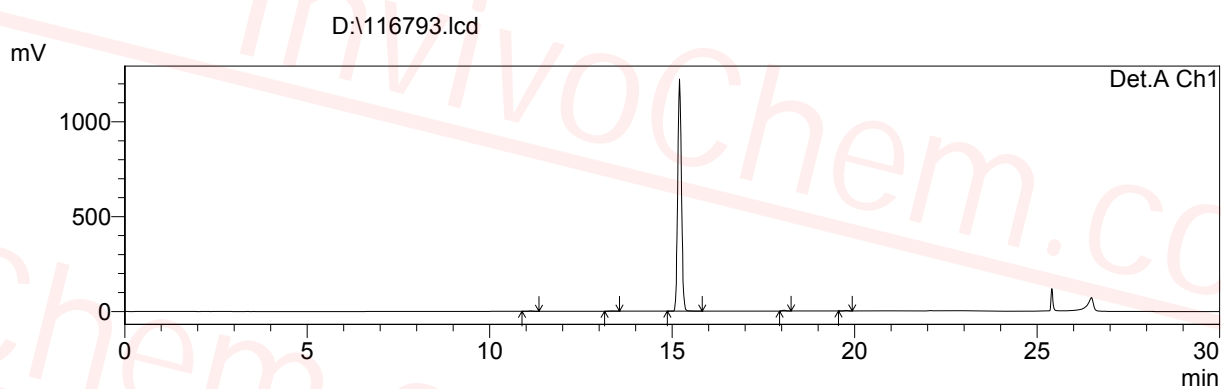

1Det.A Ch1/220nm
2Det.A Ch2/254nm

PeakTable

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Area %	Theoretical Plate#
1	11.116	12645	0.144	45115.113
2	13.351	8293	0.095	64718.714
3	15.198	8713006	99.290	93201.528
4	18.061	27282	0.311	142362.227
5	19.769	14070	0.160	198025.167

Peak#	Ret. Time	Area	Area %	theoretical Plate#
Total		8775296	100.000	

PeakTable

Detector A Ch2 254nm

Peak#	Ret. Time	Area	Area %	theoretical Plate#
1	11.115	8818	0.119	44167.726
2	13.349	5242	0.071	66953.914
3	14.325	2433	0.033	70493.715
4	15.198	7368253	99.130	92953.225
5	18.061	35591	0.479	139602.879
6	19.769	12582	0.169	184860.568
Total		7432918	100.000	

*** End Of Report ***