


V216401 C-26196 HPLC

Injection Date : 22 Mar 20
Sample Name : SC-26196
Acq. Operator : YDY
Spec. Reported : MS Integration
Acq. Method : E\1-POS-3MIN.M
Analysis Method : E\1-POS-3MIN.M
Sample Info : Easy-Access Method: '1-POS-3MIN.M' 423.00
Method Info : Mobile Phase: A:Water(10mM NH4HCO3) B:ACN
Gradient: 5% increase to 95%B within 1.4min, 95%B for 1.6min.
Flow Rate: 1.8ml/min
Column: XBridge C18,4.6*50mm,3.5um
Column Temperature: 45 C
Detection:UV(214,4nm) and MS(ESI,Neg mode,110 to 1000 amu)

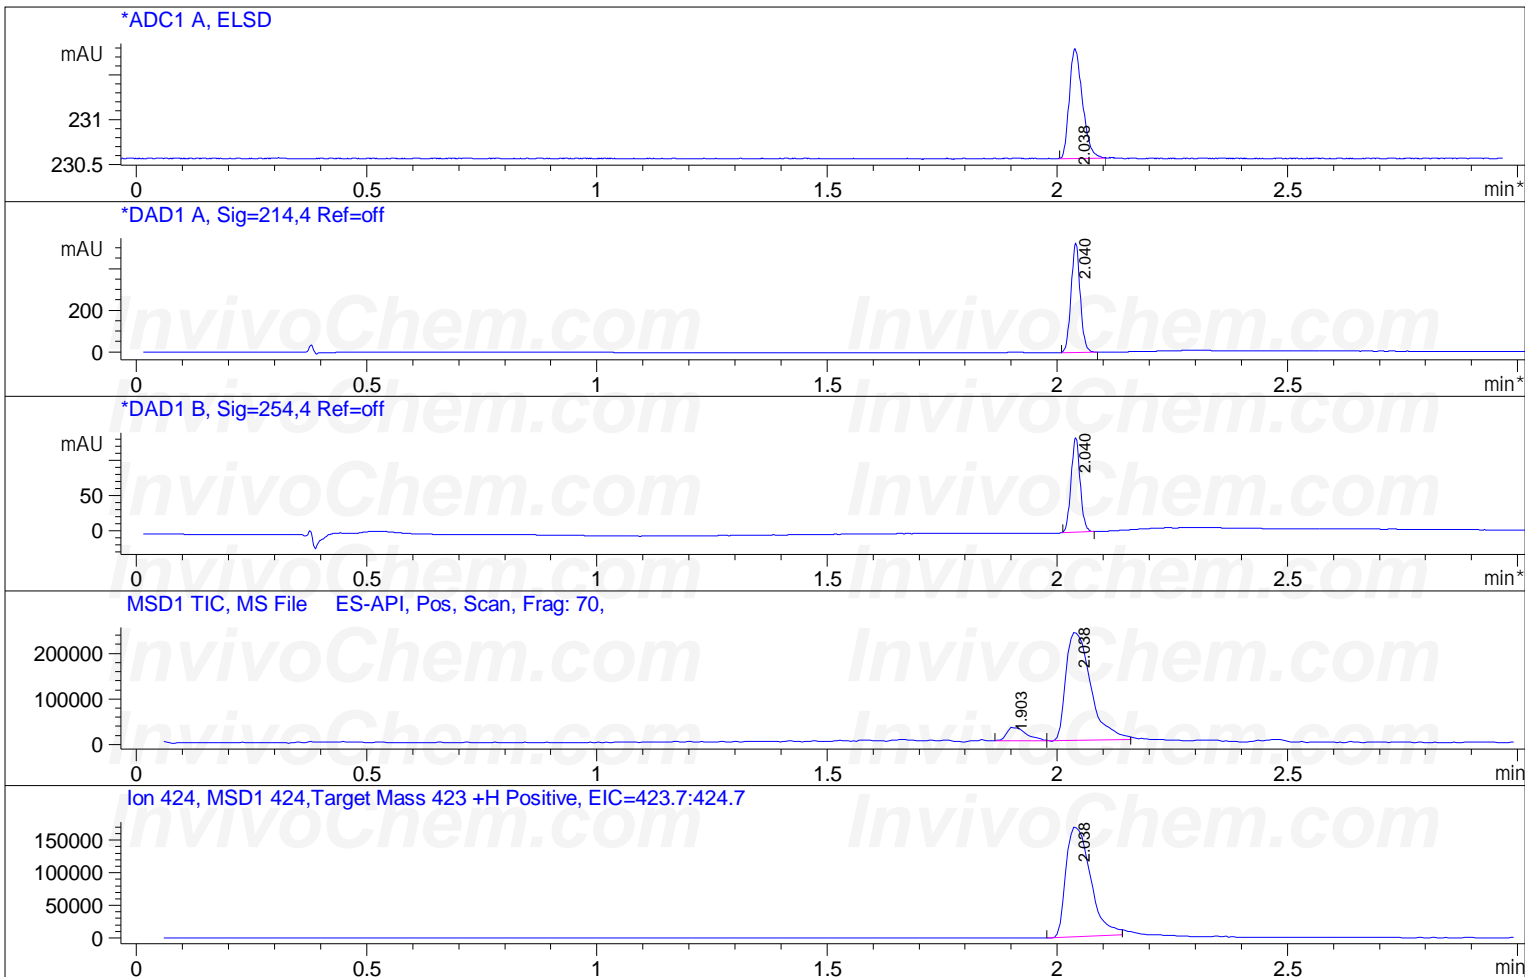

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
2.04	0.03	2.42	1.22	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
2.04	0.02	721.70	524.27	100.00


Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
2.04	0.02	182.85	133.78	100.00

V216401 C-26196 HPLC

Ret. Time: 1.90

<<<< POSITIVE SPECTRA >>>>

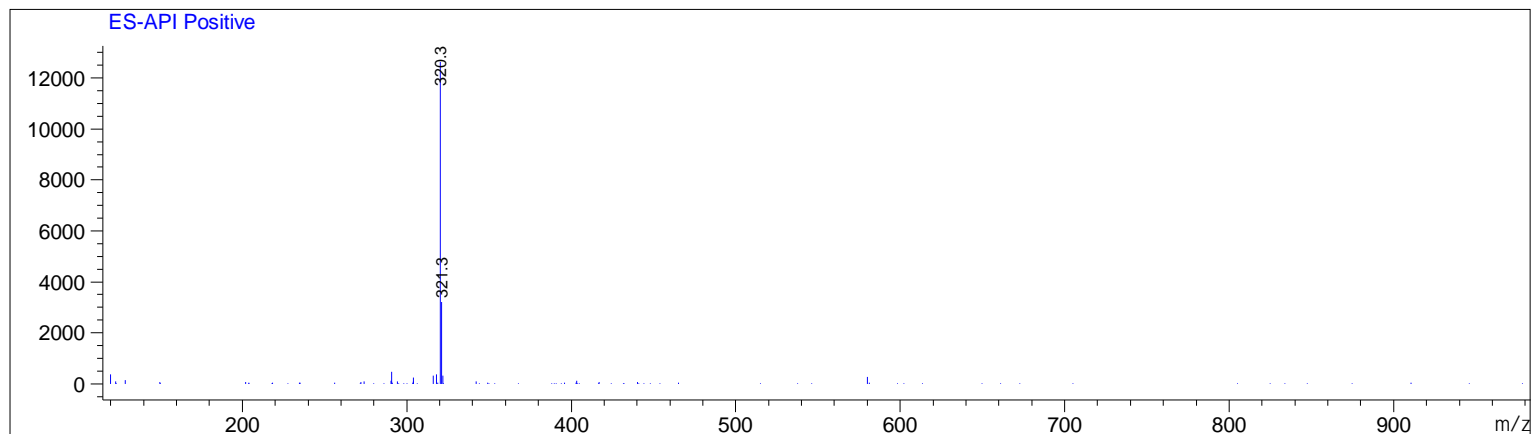

Ret. Time: 2.04

