


V1694501 TVB-2640 HPLC

=====
Acq. Operator : SYSTEM
Acq. Instrument : 12601c

Seq. Line : 6
Location : Vial 30

Inj Volume : 2.000 µl

Additional Info : Peak(s) manually integrated

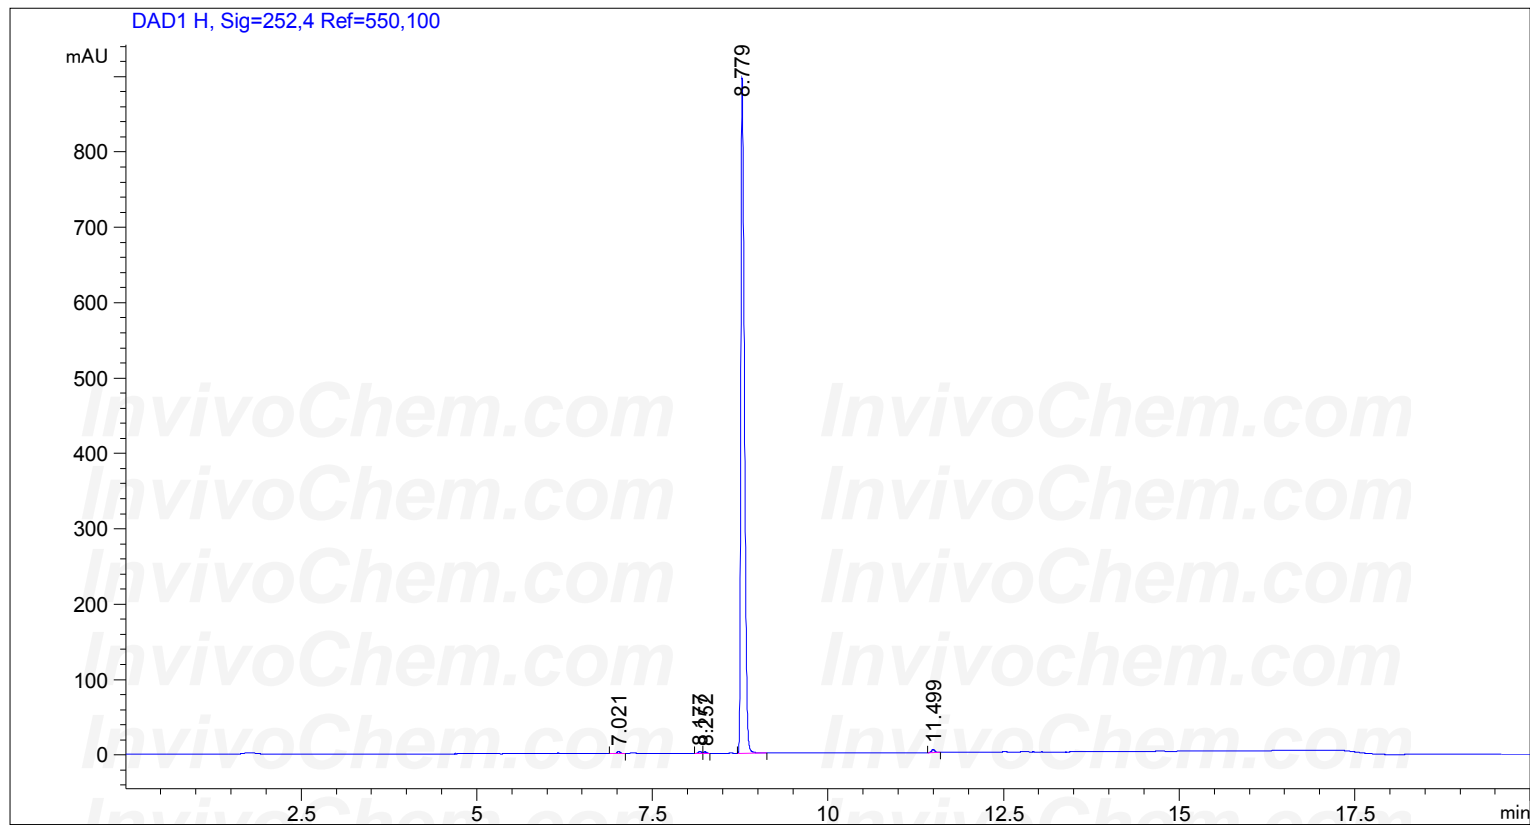

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 H, Sig=252,4 Ref=550,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	7.021	BB	0.0427	7.41868	2.64453	0.2342
2	8.177	BV	0.0451	6.78757	2.35356	0.2143
3	8.252	VB	0.0430	5.72622	2.05490	0.1808
4	8.779	BB	0.0543	3134.18262	895.71265	98.9478
5	11.499	BB	0.0492	13.39562	4.26084	0.4229

Totals : 3167.51070 907.02647

InvivoChem.com
InvivoChem.com
InvivoChem.com
InvivoChem.com
InvivoChem.com
InvivoChem.com
InvivoChem.com
InvivoChem.com

InvivoChem.com
InvivoChem.com
InvivoChem.com
Invivochem.com
InvivoChem.com
InvivoChem.com
InvivoChem.com
InvivoChem.com