


HPLC Analysis for V3415801 PAβN dihydrochloride

Data file: C:\CHEM32\1\DATA\200703\602755 20070005Final.D
Sample name: 602755 20070005Final
Description: Mobile phase: Buffer A: 0.1%TFA in H2O
Buffer B: 0.1%TFA in ACN
Gradient: 23-43% B in 20min, Flow rate: 1.0ml/min
Column: Unitary C18, 4.6*150mm, 5um 100A (A-007)
Instrument: Agilent HPLC 1100

Instrument: 1100 **Location:** 13
Injection date: 2020/7/3 13:16:24 **Injection:** 1 of 1
Last changed: 2020/7/3 14:41:31 **Injection volume:** 5.000
Acq. operator: qc

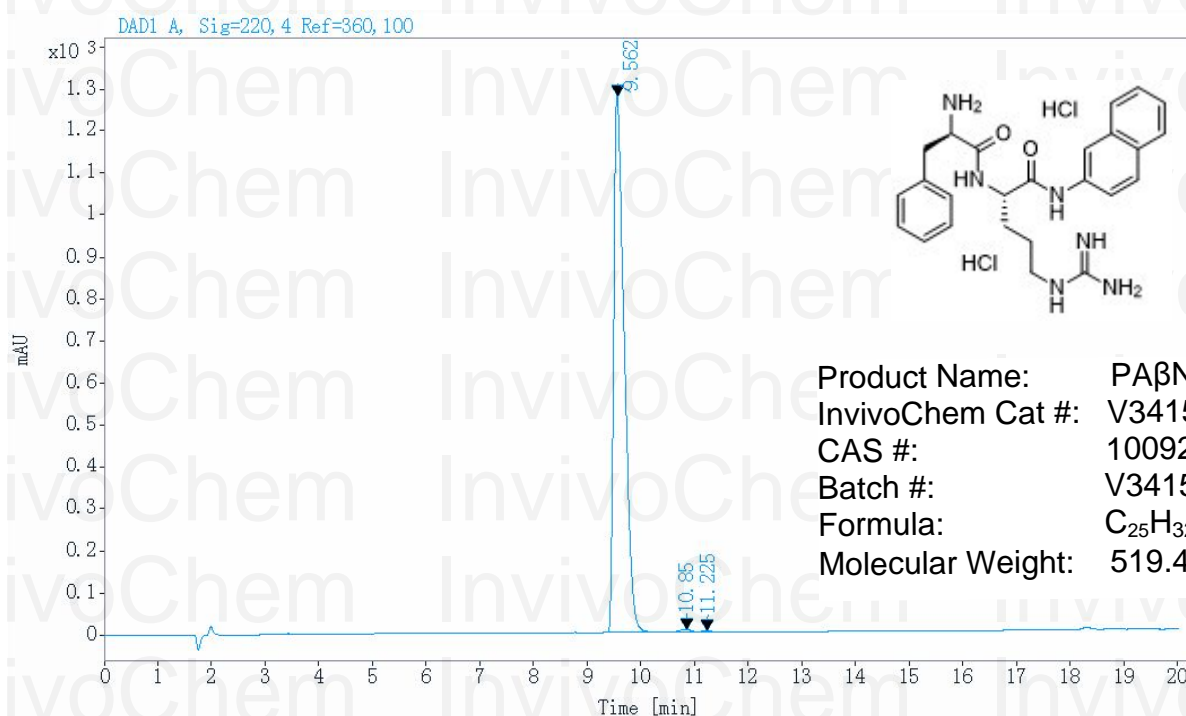

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[min]	Type	Width[min]	Area	Height	Area%	Name
9.562	BBA	0.2119	17418.3594	1270.5997	99.3627	
10.850	BV	0.2532	80.5849	5.1887	0.4597	
11.225	VB	0.1801	31.1384	2.7511	0.1776	
Sum			17530.0827			