


HPLC Analysis for V40672 4-Hydroxynonenal-HPLC

```
=====
Acq. Operator   : SYSTEM                      Seq. Line :    9
Acq. Instrument : 12601c                     Location  : Vial 100

                                           Inj Volume : 2.000 µl
=====
```

Additional Info : Peak(s) manually integrated

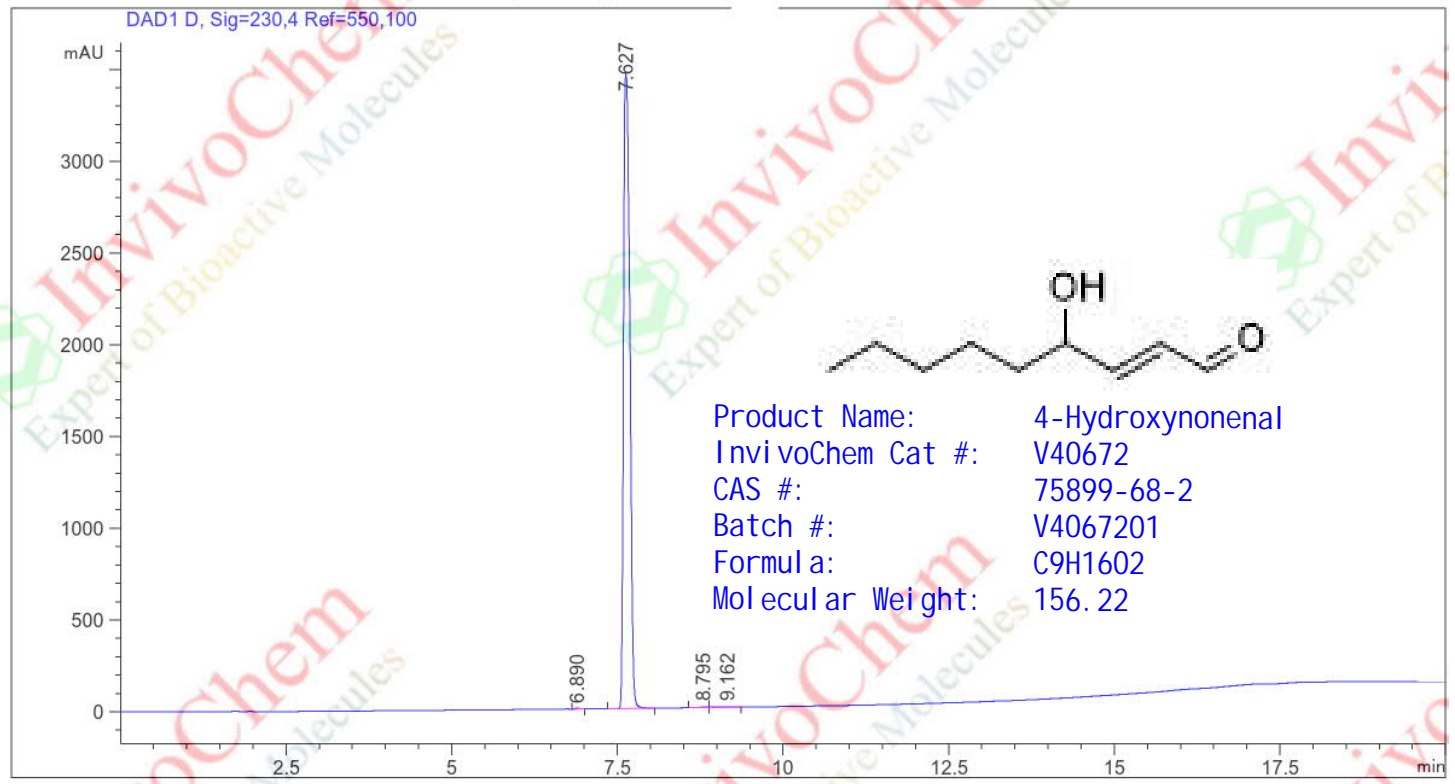

=====
 Area Percent Report
 =====

```
Sorted By      :      Signal
Multiplier     :      1.0000
Dilution       :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Signal 1: DAD1 D, Sig=230,4 Ref=550,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	6.890		0.0670	23.16859	5.00596	0.1012
2	7.627		0.0879	2.27899e4	3456.41699	99.5535
3	8.795		0.1109	20.01124	2.47299	0.0874
4	9.162		0.2401	59.03117	2.94245	0.2579
Totals :				2.28921e4	3466.83840	

*** End of Report ***