


# HPLC Analysis for V1608 Nocodazole 31430-18-9

Data File D:\DATA\2022-08-30 15-32-34\P1.D Sample

Name: P1

```

=====
Acq. Operator   : SYSTEM                               Seq. Line :    7
Acq. Instrument : PAS-HPLC-0013                       Location  : Vial 42
Injection Date  : 8/30/2022 4:33:39 PM                Inj       :    1
                                                    Inj Volume: 1.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 0.500 µl
Acq. Method     : D:\DATA\2022-08-30 15-32-34\5-90-TFA-214NM-PROCELL-50.M
Last changed    : 8/30/2022 3:32:36 PM by SYSTEM
Analysis Method : D:\DATA\2022\20220824 2022-04-28 09-56-09\5-90-TFA-214NM-PROCELL-50.M
(
                Sequence Method)
Last changed    : 8/28/2022 9:56:10 AM by SYSTEM
    
```

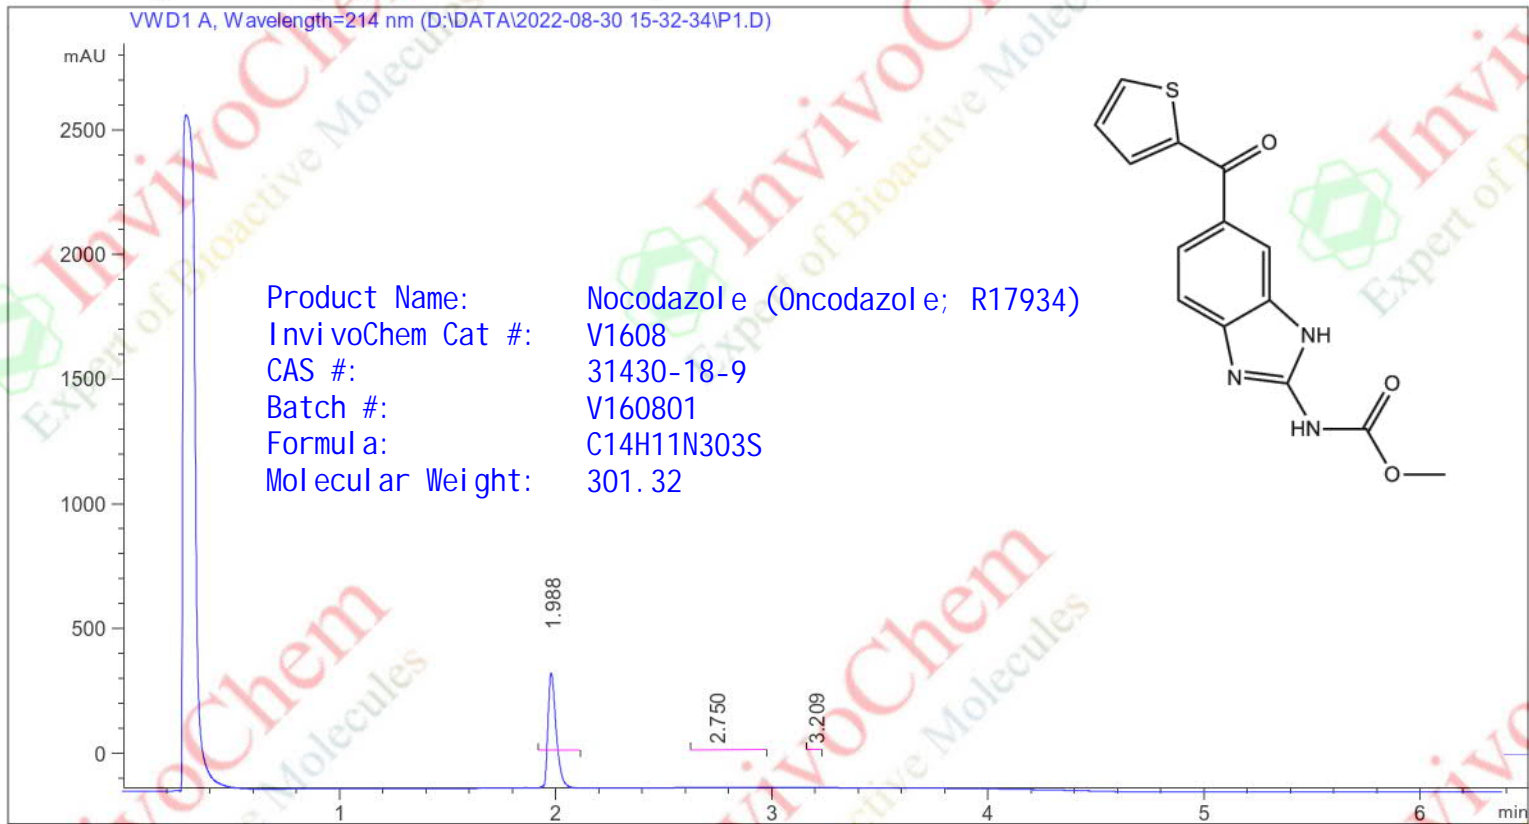

## Area Percent Report

```

Sorted By      : Signal
Multiplier     : 1.0000
Dilution       : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs
    
```

Signal 1: VWD1 A, Wavelength=214 nm

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.988	VV	0.0408	1222.04028	462.32181	98.9440
2	2.750	VB	0.0736	12.27056	2.08642	0.9935
3	3.209	BV	0.0342	7.71646e-1	3.13397e-1	0.0625
Totals :				1235.08249	464.72163	

=====  
\*\*\* End of Report \*\*\*